

Alcotest 7110 Calibration Record

Equipment

Alcotest 7110 MKIII-C
Location: BLAIRSTOWN POLICE DEPT. Serial No.: ARWE-0027
Calibration File No.: 00129 Calib. Date: 04/03/2009 Calib. No.: 00008
Certification File No.: 00111 Cert. Date: 10/30/2008 Cert. No.: 00005
Linearity File No.: 00112 Lin. Date: 10/30/2008 Lin. No.: 00005
Solution File No.: 00128 Soln. Date: 03/18/2009 Soln. No.: 00055
Sequential File No.: 00129 File Date: 04/03/2009


Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWH S3-0284
Control Solution %: 0.100% Expires: 07/02/2010
Solution Control Lot: 08G056 Bottle No.: 1379

Coordinator

Last Name: ROUSHINKO First Name: CRAIG MI: A.
Signature: TPR. II C.R. #6046 Badge No.: 6046
Date: 04/03/2009

*Black Key Temperature Probe Serial.....# DDWAP2-038 CAR

*Digital NIST Temperature Measuring System Serial.....# 80614942 CAR

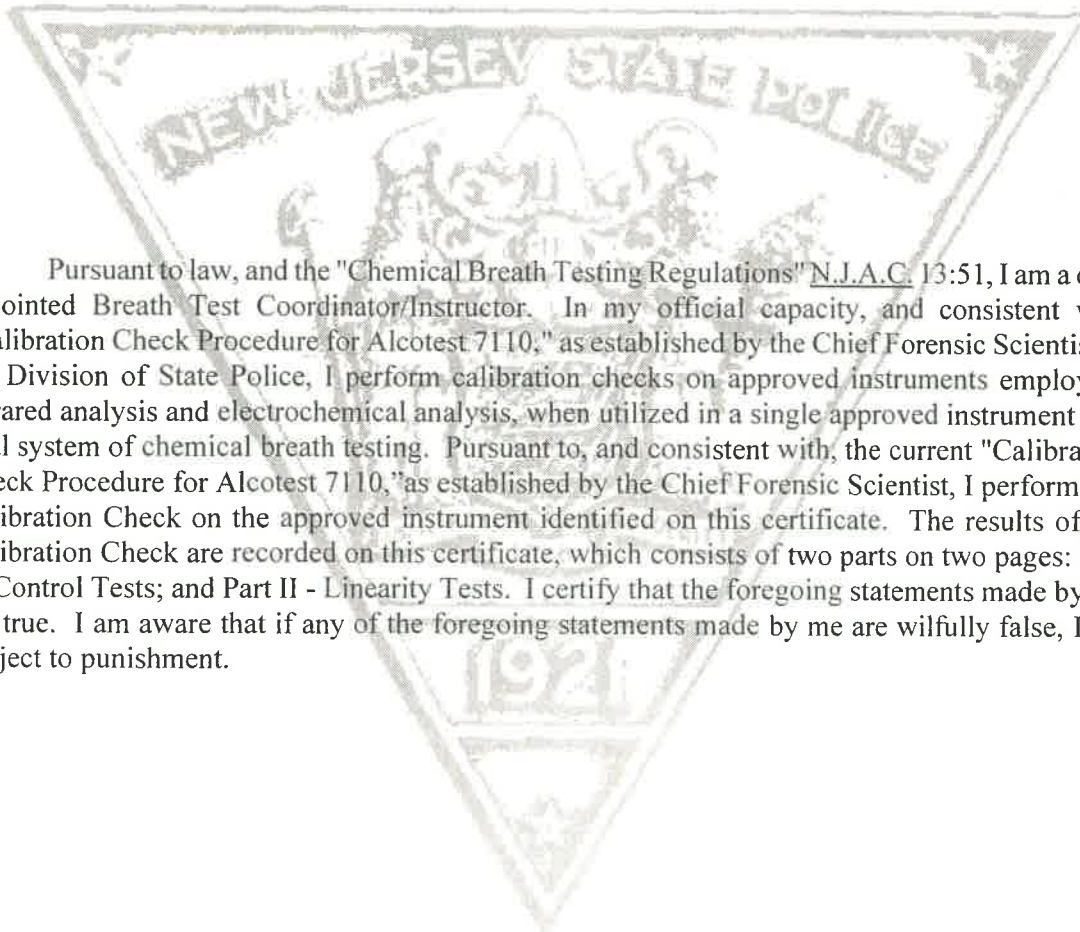

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWE-0027
Location:	BLAIRSTOWN POLICE DEPT.	
Calibration File No.:	00129	Calib. No.: 00008
Certification File No.:	00130	Cert. Date: 04/03/2009
Linearity File No.:	00112	Cert. No.: 00006
Solution File No.:	00128	Lin. Date: 10/30/2008
Sequential File No.:	00130	Lin. No.: 00005
		Soln. No.: 00055
		File Date: 04/03/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWH S3-0284
Solution Control Lot:	08G056	Expires: 07/02/2010
		Bottle No.: 1379

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:19S	34.0°C	
Control 1 EC	0.100%	12:20S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	12:20S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:21S		
Control 2 EC	0.100%	12:21S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	12:21S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:22S		
Control 3 EC	0.099%	12:23S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	12:23S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:23S		

All tests within acceptable tolerance.

Coordinator

Last Name: ROUSHINKO First Name: CRAIG MI: A.
 Signature: TR II C. R. #6046 Badge No.: 6046 Date: 04/03/2009

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARWE-0027
 Location: BLAIRSTOWN POLICE DEPT.
 Calibration File No.: 00129 Calib. Date: 04/03/2009 Calib. No.: 00008
 Certification File No.: 00130 Cert. Date: 04/03/2009 Cert. No.: 00006
 Linearity File No.: 00131 Lin. Date: 04/03/2009 Lin. No.: 00006
 Solution File No.: 00128 Soln. Date: 03/18/2009 Soln. No.: 00055
 Sequential File No.: 00131 File Date: 04/03/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDRK S3-0021
 Control Solution %: 0.040% Expires: 06/26/2010
 Solution Control Lot: 08F054 Bottle No.: 0337

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDRK S3-0022
 Control Solution %: 0.080% Expires: 06/28/2010
 Solution Control Lot: 08F055 Bottle No.: 0164

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDRK S3-0024
 Control Solution %: 0.160% Expires: 07/07/2010
 Solution Control Lot: 08G057 Bottle No.: 1307

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:37S	13:37 D (CAL)	
Control 1 EC	0.042%	12:38S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.040%	12:38S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:39S		
Control 2 EC	0.041%	12:40S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.039%	12:40S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:41S		
Control 3 EC	0.081%	12:42S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.078%	12:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:44S		
Control 4 EC	0.081%	12:44S	34.0°C	*** TEST PASSED ***
Control 4 IR	0.078%	12:44S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:46S		
Control 5 EC	0.161%	12:46S	34.0°C	*** TEST PASSED ***
Control 5 IR	0.160%	12:46S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:48S		
Control 6 EC	0.159%	12:49S	34.0°C	*** TEST PASSED ***
Control 6 IR	0.159%	12:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:50S	13:50 D (CAL)	

All tests within acceptable tolerance.

Coordinator

Last Name: ROUSHINKO

First Name: CRAIG

MI: A.

Signature: TRE II C [Signature] #6046

Badge No.: 6046

Date: 04/03/2009

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWE-0027
Location:	BLAIRSTOWN POLICE DEPT.	
Calibration File No.:	00129	Calib. Date: 04/03/2009
Certification File No.:	00130	Calib. No.: 00008
Linearity File No.:	00131	Cert. Date: 04/03/2009
Solution File No.:	00132	Cert. No.: 00006
Sequential File No.:	00132	Lin. Date: 04/03/2009
		Lin. No.: 00006
		Soln. Date: 04/03/2009
		Soln. No.: 00056
		File Date: 04/03/2009

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDWH S3-0284
Control Solution %: 0.100%		Expires: 03/07/2010
Solution Control Lot: 08C051		Bottle No.: 0955

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:57S	14:57 D (CAR)	
Control 1 EC	0.100%	13:58S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	13:58S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:59S		
Control 2 EC	0.099%	13:59S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	13:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:00S		
Control 3 EC	0.099%	14:01S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	14:01S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:01S	15:01 D (CAR)	

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DPWAP2-008 (CAR)

Changed By:

Last Name: ROUSHINKO

First Name: CRAIG

MI: A.

Signature: TPR II C. D. #6046

Badge No.: 6046

Date: 04/03/2009

Drägersafety

Alcotest[®] 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

05/01/2007

SERIAL NUMBER:

ARWE-0027

Draeger Safety Diagnostics, Inc.
Durango, CO

CRD