

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWE-0027
Location:	BLAIRSTOWN POLICE DEPT.	
Calibration File No.:	00148	Calib. Date: 09/28/2009
Certification File No.:	00149	Cert. No.: 00009
Linearity File No.:	00150	Cert. Date: 09/28/2009
Solution File No.:	00155	Lin. No.: 00007
Sequential File No.:	00155	Lin. Date: 09/28/2009
		Soln. No.: 00067
		Soln. Date: 11/22/2009
		File Date: 11/22/2009

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDWH S3-0283
Control Solution %: 0.100%		Expires: 03/07/2010
Solution Control Lot: 08C051		Bottle No.: 0956

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:55S		
Control 1 EC	0.099%	11:56S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	11:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:57S		
Control 2 EC	0.100%	11:57S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	11:57S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:58S		
Control 3 EC	0.100%	11:59S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	11:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:59S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: FALCICCHIO

First Name: NICHOLAS

MI: -

Signature: \_\_\_\_\_

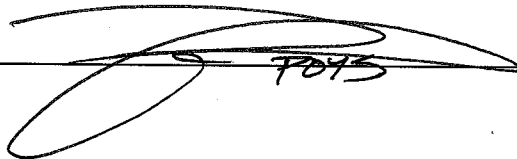

Badge No.: 45

Date: 11/22/2009