

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWE-0027
Location: BLAIRSTOWN POLICE DEPT.
Calibration File No.: 00148 Calib. Date: 09/28/2009 Calib. No.: 00009
Certification File No.: 00149 Cert. Date: 09/28/2009 Cert. No.: 00007
Linearity File No.: 00150 Lin. Date: 09/28/2009 Lin. No.: 00007
Solution File No.: 00156 Soln. Date: 12/17/2009 Soln. No.: 00068
Sequential File No.: 00156 File Date: 12/17/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWH S3-0283
Control Solution %: 0.100% Expires: 03/07/2010
Solution Control Lot: 08C051 Bottle No.: 0973

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:50S		
Control 1 EC	0.100%	18:51S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	18:51S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:52S		
Control 2 EC	0.100%	18:52S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	18:52S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:53S		
Control 3 EC	0.101%	18:54S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	18:54S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:55S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: DALRYMPLE

First Name: KYLE

MI: B

Signature: _____

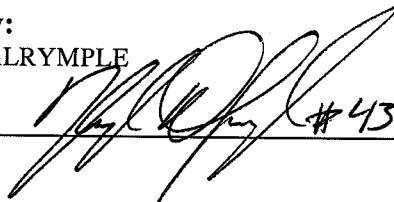

Badge No.: 43

Date: 12/17/2009